

# Güralp Artius

## *Technical Manual*

*Document Number: MAN-ART-0001*

*10/02/2026 12:08:48*

---

*Designed and manufactured by*  
Güralp Systems Limited  
3 Midas House, Calleva Park  
Aldermaston RG7 8EA  
England

---

# Table of Contents

---

<b>1. Preliminary Notes</b>	<b>5</b>
1.1. Proprietary Notice	5
1.2. Notes Cautions and Warnings	5
1.3. Manuals and Software	5
1.4. Conventions	5
<b>2. Overview</b>	<b>7</b>
2.1. Key Features	7
2.2. Typical Applications Examples	8
2.3. System Description	8
2.3.1. Digital Broadband Node	8
2.3.2. Internal GNSS	8
2.3.3. Single Connector	8
2.3.4. LED indicator	8
2.3.5. Bluetooth Connectivity	9
2.3.6. MEMS Accelerometer	9
2.3.7. Data Storage	9
2.4. Package Content	9
2.4.1. Artius Seismic Node	10
2.4.2. Power-Data Cable	10
2.4.3. Docking Station (Optional)	10
2.4.4. Power Pack Module (Optional)	10
2.4.5. Deployment Feet or Spikes (Optional)	11
2.5. Companion Software	12
2.5.1. Discovery	12
2.5.2. Web Interface	12
2.5.3. GüVü	13
<b>3. Configuration</b>	<b>14</b>
3.1. Physical Setup	14
3.2. Access the Web Interface	15
3.2.1. Finding the Artius with Discovery	15

---

3.2.2. Logging In	15
3.3. Web Interface Overview	17
3.4. Station Metadata	17
3.5. Timing Options	18
3.5.1. GNSS lock status	18
3.5.2. NTP (Network Timing Protocol) configuration	19
3.6. Data Transmission	19
3.7. Data Recording	21
3.8. Earthquake Early Warning	22
3.8.1. Trigger Configuration	22
3.8.2. CAP receiver	24
3.8.3. STA/LTA Streams	24
3.8.4. Seismic Event Table	24

---

## **4. Data Access** **26**

4.1. Seismic and SOH miniSEED files	26
4.1.1. Data download: Discovery's Docking Station Tool	26
4.1.2. Bulk Data Download via Webpage	26
4.1.3. Time-Based Data Download via Webpage	27
4.1.4. Bulk Data Extraction via Network	28
4.1.5. Time Based-Data Extraction via Network	29
4.2. Metadata	31
4.2.1. RESPonse Files	31
4.2.2. Station XML Files	32
4.2.3. Dataless SEED Volume	33

---

## **5. Bluetooth Connectivity: the GüVü App** **34**

5.1. Getting Stated	34
5.2. View Settings	35
5.3. Instrument Control	35
5.3.1. Setting the PIN Code	37
5.4. Emailing a Deployment Report	37

---

## **6. Firmware Update** **39**

<b>7. Installation</b>	<b>41</b>
7.1. Direct Burial with PPM	41
7.2. Surface Deployment with Spike	42

---

<b>8. Appendices</b>	<b>44</b>
8.1. Connector Pin-Outs	44
8.2. Network Ports	44
8.3. Channel Names	45

# 1. Preliminary Notes

## 1.1. Proprietary Notice

The information in this document is proprietary to Güralp Systems Limited and may be copied or distributed for educational and academic purposes but may not be used commercially without permission.

Whilst every effort is made to ensure the accuracy, completeness, and usefulness of the information in the document, neither Güralp Systems Limited nor any employee assumes responsibility or is liable for any incidental or consequential damages resulting from the use of this document.

## 1.2. Notes Cautions and Warnings

Note Cautions and Warnings are displayed and defined as follows:



**Note:** Indicates a procedural or advisory information



**Caution:** Highlights a condition or action that, if not followed, may result in equipment damage, reduced performance, or loss of data.



**Warning:** Alerts to a hazard that could result in personal injury or serious damage to the equipment if ignored.

## 1.3. Manuals and Software

All manuals and software referenced in this document are, unless stated otherwise, available from the Güralp Systems Ltd website: [www.guralp.com](http://www.guralp.com).

## 1.4. Conventions

Throughout this manual, examples of command-line interactions are shown in a fixed-width typeface:

fixed-width example

Commands you must type appear in **bold**:

**bold fixed-width example**

Variable elements you must replace with values specific to your configuration are blue and shown in bold:

**Blue blue fixed-width example**

## Güralp Artius

Putting these together into a single example:

System prompt: **User input** **variable parameter**

On-screen buttons referenced in procedures are shown using the following style:

**Example Button**

## 2. Overview

Thank-you for purchasing the Güralp Artius broadband node.

The Güralp Artius is an advanced, ultra-compact 3-component digital broadband seismic node designed for rapid, high-density seismic deployments. It features internal 24-bit digitiser, GNSS, Bluetooth and miniSEED output.



### 2.1. Key Features

- Digital, three-axis, broadband, force-feedback seismometer.
- Flat response to ground acceleration from 30 s to 200 Hz.
- Standard gain equivalent to 500 V/ms<sup>-1</sup>.
- Selectable sample rates from 1 to 1000 samples per second.
- Compact form, measuring just 80 × 80 × 105 mm<sup>3</sup> and 1.4 kg weight.
- Single port for connection to power supply and docking station.
- Internal ±2 g MEMS accelerometer for orientation.
- Identification of IP address via Güralp Discovery software and docking station.
- Optional docking station (fits up to 8 Artius) for configuration and data handling operations.
- Android app for installation integrity checking via Bluetooth.
- Data storage with 64 GB microSD card (option of 128 GB).
- In-built GNSS receiver, compatible with GPS, GLONASS and Galileo constellations (BeiDou optional).
- Optional Power Pack Module (PPM) with rechargeable lithium batteries and integrated charge controller.

---

## 2.2. Typical Applications Examples

- Network densification
  - Temporary seismic investigations
  - Rapid response
  - High resolution imaging
  - Microseismic monitoring
  - Aftershock studies
  - Environmental and induced seismicity monitoring
- 

## 2.3. System Description

---

### 2.3.1. Digital Broadband Node

The Güralp Artius is a broadband triaxial seismometer integrated with a Minimus Lite digitiser front end. The Minimus Lite acquires data from the instrument and provides direct control of its operation.

---

### 2.3.2. Internal GNSS

The in-built GNSS receiver supports the GPS, GLONASS and Galileo satellite constellations, with BeiDou as an option. The top panel of the Artius is made of tempered glass to provide the GNSS receiver with an unobstructed view of the sky for signal acquisition.

---

### 2.3.3. Single Connector

The Artius is equipped with a single connector on the rear panel, which supplies power and supports communication via an M12 Automation Connector (Decoding M12).



---

### 2.3.4. LED indicator

Artius units have an LED indicator on the top, which provides status and configuration information.

When powered-up, the Artius' LED will indicate its status. After the startup - during which the LED is white ● - the LED repeats a sequence of three flashes, followed by a pause:

- Flash 1: SD card status
- Flash 2: Centring sensor status
- Flash 3: GPS time lock

Each flash is either:

- Green ●: Status OK / good GPS lock
- Red ●: Status error / no GPS lock

The LED flashing blue ● indicates active data offload.

Example:



SD card is recording, sensors are centred, but lock to GNSS has not been achieved.

### 2.3.5. Bluetooth Connectivity

The Artius features Bluetooth connectivity, allowing sensor and state-of-health data to be monitored using the Güralp GüVü app running on an Android mobile phone or tablet.

Bluetooth can be disabled via software to save processing power, but the hardware module cannot be switched off. BLE (Bluetooth Low Energy) technology is used to minimise the power requirement. The Bluetooth transmitter/receiver is in permanent standby mode and always ready to receive a connection from a phone or tablet.

### 2.3.6. MEMS Accelerometer

The Artius is equipped with a triaxial Micro Electro-Mechanical System (MEMS) accelerometer with a measurement range of  $\pm 2$  g. The three axes of sensitivity, Z, N and E, align with those of the main seismometer outputs.

### 2.3.7. Data Storage

The Artius uses a microSD card to store seismic data within the instrument. The microSD card is internal and cannot be removed by the user. The standard storage capacity is 64 GB, but it can be increase to 128 GB upon request when placing the order. Data is recorded in miniSEED format, while metadata is stored in dataless SEED, Station XML and RESP files.

## 2.4. Package Content

The Artius package includes:

- Artius seismic node
- Artius power-data cable
- Docking Station with power cable (optional)
- Accessories, such as Power Pack Module, deployment feet or spikes (optional)

---

### 2.4.1. Artius Seismic Node

Description in Section 2.3.

---

### 2.4.2. Power-Data Cable


The Artius comes with a dedicated power-data cable with a M12-D-Coded automation connector on one end and bare ends at the other. The power-data cable connects to the single connector on the Artius' rear panel (see Section 2.3.3)

Pin-out details are provided in Section 8.1.

---

### 2.4.3. Docking Station (Optional)

The Docking Station supports up to 8 Artius nodes, optimising both pre-deployment configuration and post-deployment data transfer. The Artius nodes are inserted vertically and slide into place.

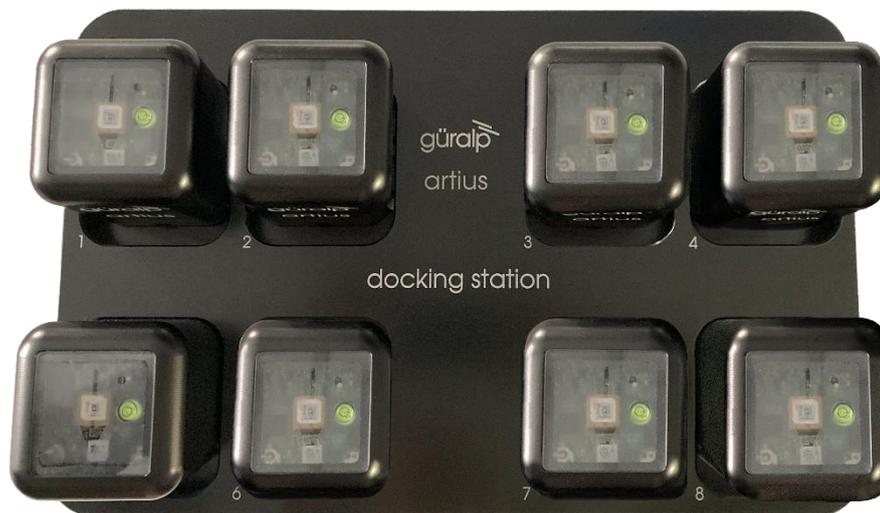

The docking station provides power to each Artius units, so no external power supply is required. The docking station is connected to power through a single connector.

Two separate Ethernet ports on the rear of the Docking Station provide access to slots 1-4 and 5-8. When used in conjunction with our Discovery application a dedicated interface streamlines configuration and data download. An Ethernet switch, or similar equipment, is required to connect both rows of the Docking Station simultaneously.

---

### 2.4.4. Power Pack Module (Optional)



The Güralp Power Pack Module (PPM) is a smart charge-controller and battery system that can provide continuous power to an Artius unit. It can be used either as a stand-alone battery for short-term, off-grid deployments or as power source in a solar-powered installation. When used with solar panels, the integrated charge controller operates on the MPPT (Maximum Power Point Tracking) principle to continuously adjust its input impedance to draw the maximum power from the connected solar panel, under varying light conditions.



**Note:** Please refer to the [Power Pack Module manual](#) for more details and user instructions.

---

### 2.4.5. Deployment Feet or Spikes (Optional)

The Artius can be supplied with deployment feet, one spike or three smaller spikes to suit various styles of deployment and types of terrain. The recommended setup of the Artius is described in Section 7.1 and involves burying the instrument along with the connected cable and power supply. This helps to mitigate noise generated by the local environment and provide better coupling.

Should the ground be too hard or hazardous to dig into, the 250mm or 162mm spike(s) can be attached to the Artius to secure it firmly while leaving the instrument at the surface.

Artius may be deployed on its standard feet in environments which have already been shielded from local noise and coupled to the ground, such as on top of a concrete base of a

seismic station. In this setting, the instrument may also be placed in a box and surrounded by sand for additional coupling and thermal insulation.



---

## 2.5. Companion Software

This section introduces the Güralp software available for interacting with Minimus.

---

### 2.5.1. Discovery

Güralp's Discovery software for Windows and Linux allows users to configure instruments, monitor state-of-health, view waveforms, acquire data and perform analysis on live or recorded data via filtering or creating plots - such as a PSD or Spectrogram. It can locate instruments on a local network and, when configured, enable remote access to networked instruments in the field.



**Note:** Comprehensive guidance for Discovery is beyond the scope of this document, see the full Discovery manual: [MAN-DIS-0001](#).

---

### 2.5.2. Web Interface

The Artius hosts a web server accessible via any browser, providing a user-friendly interface for monitoring and configuration. Users can view sensor readings, adjust parameters, manage data streaming, and access data retrieval tools. This webpage is accessible by right-clicking the Artius entry in Discovery. Selecting the (in system browser) will open the webpage in the user's default browser and is recommended for ease of downloading data.

Status	Label	System	Name	SEED Name	Site Name	Firmware Ver	(Identifier)
  	Artius_200Hz	Artius	ART-6CF6	DG.06CF6	No site	2.1-2776	(ART-6CF6)
<div style="border: 1px solid gray; padding: 5px;"> <p style="text-align: center; margin: 0;"><b>ART-6CF6</b> 10.20.0.22</p> <ul style="list-style-type: none"> <li>View Web Page <span style="float: right;">W</span></li> <li style="background-color: #e0e0e0;">View Web Page (in system browser)</li> <li>Show On Map</li> <li>Console <span style="float: right;">C</span></li> <li>Live View <span style="float: right;">▶</span></li> <li>Offload View <span style="float: right;">▶</span></li> <li>Get Manual <span style="float: right;">M</span></li> <li>Get Release Notes <span style="float: right;">R</span></li> <li>System Configuration</li> <li>Device Port Configuration</li> <li>Edit Network Address</li> <li>File Exchange</li> <li>Quick File Upload <span style="float: right;">Q</span></li> <li>Tunnel Status</li> <li>Calibration <span style="float: right;">▶</span></li> </ul> </div>							

### 2.5.3. GüVü

The GüVü Android app enables monitoring and control of nearby instruments via Bluetooth, particularly useful for verifying post-deployment configurations in the field. Instructions for using GüVü are provided in Section 5 of this manual.

## 3. Configuration



**Note:** Güralp strongly recommends exploring and familiarising yourself with the Artius in a controlled environment, such as your lab or office, before deploying it in the field.


### 3.1. Physical Setup

First connect the Docking Station, described in Section 2.4.3, to power using the mains-12VDC cable provided. The Artius slots into one of the 8 provided slots along the white rails and into the power and data port. The Artius should sit firmly in the Docking Station. Once connected, the Artius' LED will start flashing with the sequence described in Section 2.3.4.



**Note:** A full 3D GPS lock requires a clear view of the sky and may not be achievable when the device is operated indoors or in areas with significant obstructions. Even with an unobstructed view of the sky, the GPS receiver may require up to 15 minutes after initial power-up to acquire a stable 3D satellite lock on the Artius.

Connect to correct ethernet port of the Docking Station to an ethernet switch configured to your local network or directly to your laptop/PC.

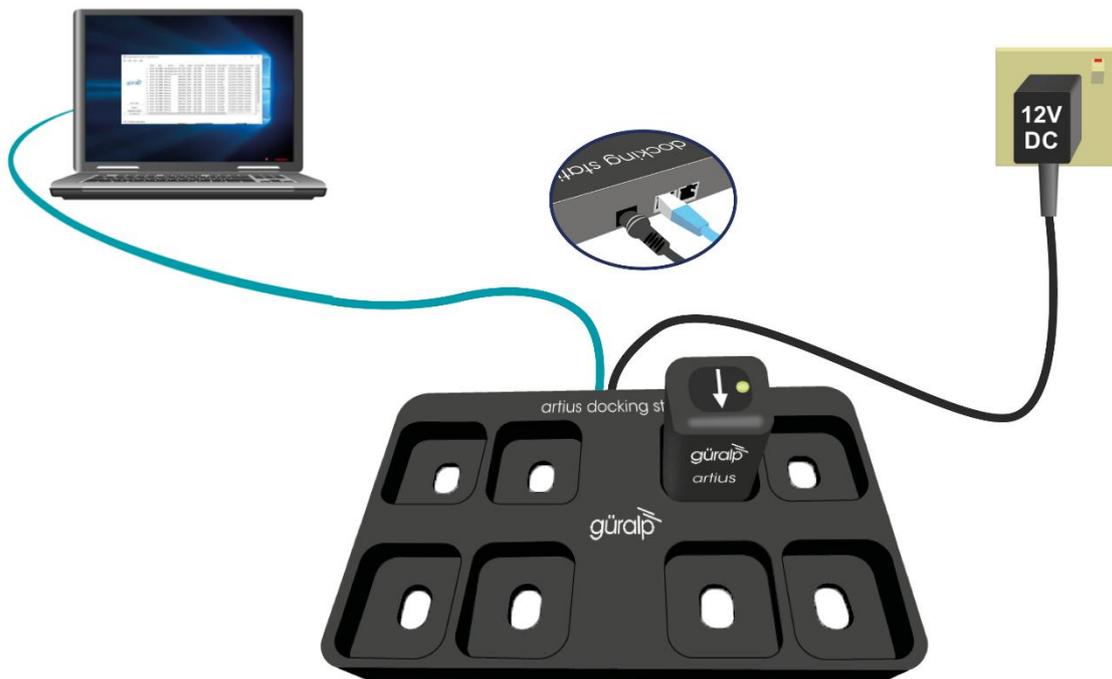

The Artius will appear as an entry in Discovery.

Güralp Systems - Discovery							
File Edit Tools Window Help Manuals							
	Status	Label	System	Name	SEED Name	Site Name	Firmware Ver
<input type="checkbox"/>	  	AGU	Artius	ART-433C	DG.0433C	No site	2.1-2656



**Note:** If the Artius does not appear in Discovery, try connecting the Ethernet cable to the other Ethernet port on the rear of the Docking Station, as each port services a different instrument row.

## 3.2. Access the Web Interface

By default, the Artius uses DHCP (Dynamic Host Configuration Protocol) to obtain an IP address. If no DHCP server is available, the Artius will fall back to a link-local (APIPA) address in the range 169.254.0.1 to 169.254.255.254 with a subnet mask of 255.255.0.0. In this case, a directly connected laptop configured for DHCP will also assign itself an APIPA address, allowing direct communication without additional network configuration.

### 3.2.1. Finding the Artius with Discovery

Once the Artius and your laptop are on the same subnet, opening Discovery will list all Güralp devices on the local network. To refresh the list, click the **Scan locally** button in the bottom left corner.

### 3.2.2. Logging In

To access the Artius web interface, right click its entry in Discovery and select 'View Web Page', the (in system browser) option is recommend for ease of downloading data.

	Status	Label	System	Name	SEED Name	Site Name	Firmware Ver	(Identifier)
<input checked="" type="checkbox"/>	  	Artius_200Hz	Artius	ART-6CF6	DG.06CF6	No site	2.1-2776	(ART-6CF6)

**ART-6CF6** 10.20.0.22

- View Web Page W
- View Web Page (in system browser)
- Show On Map
- Console C
- Live View ▶
- Offload View ▶
- Get Manual M
- Get Release Notes R
- System Configuration
- Device Port Configuration
- Edit Network Address
- File Exchange
- Quick File Upload Q
- Tunnel Status
- Calibration ▶

This will open the webpage on the Status tab. Use the Login option to access further information and functionalities.

**System type: Artius | Host label: Artius\_200Hz | Host name: ART-6CF6 (10.20.0.22) | Serial number: 06CF6**

General Status					
Host name	ART-6CF6	Host label	Artius_200Hz	System type	Artius
Serial number	06CF6	Firmware version	2.1-2776	IPv4 address	10.20.0.22 (DHCP)
Digitiser temperature	41.051 °C	Digitiser humidity	27.73%	Input voltage	0.000 V
System time	2:08:36 PM Tue 27-Jan-2026	Uptime	7m 20s	Restart Status	Restarts:376 Crashes:67 Power:121
Sensor0 serial			SEED network and station	Power over Ethernet voltage	ETH status
			DG.06CF6 (No site)	10.450 V	sckt: 0/0 data: 0/6

GNSS Status			
GNSS connection status	Connected	Last timestamp	2026-01-27 14:08:36
Last lock time	2026-01-27 14:02:50	GNSS stability	100%
Latitude	51.36077	Longitude	-1.1635
Altitude	125.1	Horizontal dilution of precision	1.13
GNSS PPS status	Trusted Pulsing	GNSS NMEA stream	Input OK
GNSS Lock state	3D locked	Number of satellites	Used: 12 In view: 1

Data Record Status					
microSD status	Recording	microSD total	60817408 KiB	microSD used	10103884 KiB
		microSD free	84%		

Güralp Systems Limited  
Midas House, Calveva Park, Aldermaston, Reading, RG7 8EA, UK  
Tel: +44 118 981 9056, Fax: +44 118 981 9943  
E-Mail: sales@guralp.com, support@guralp.com

This will open the login page.

Required fields are marked \*

Username: \*

Password: \*

Login

The Minimus web interface provides two levels of access: **administrator** and **user**. Each level has default credentials as follows:

Access Level	Username	Password	Description
User	user	user	Limited access to core settings. Configuration controls are restricted.
Admin	admin	admin	Full access to all configuration settings, including network, setup, and sensor parameters.

**Note:** For regular use and basic configuration changes, Güralp suggests logging in as **user**. Log in as **admin** only if necessary to unlock features only available in the administrator account.

### 3.2.2.1. Changing Default Credentials

After logging in as an administrator, you can manage web access options from the **Network** page. Here, you can select whether the web interface should always prompt for login or allow automatic access as the user account with the **Web Login** drop down.

Webpage access configuration					
Web Login	Not Required ▾	Username (Normal)	user	Password (Normal)	*****
Web Timeout	Not Required	Username (Admin)	admin	Password (Admin)	*****
	Required			HTTP Port	80
				Map Source	OpenStreetMaps ▾

**Network Timing**

The same menu also provides controls for changing the **username** and **password** of both the user and administrator accounts. Updating these credentials is strongly recommended to improve security.

## 3.3. Web Interface Overview

The Minimus web interface is organised into several main pages, each providing access to settings and functions. The list below gives a brief overview of the purpose of each page:

1. **Status:** Displays the current operational state of the device, including sensor firmware version, humidity and temperature, GNSS status, SD card state, etc. Use this page to monitor the overall health of your Artius station.
2. **Network:** Provides configuration options for basic and advanced networking features, as well as control over security settings and timing sources.
3. **Setup:** Allows configuration of the station's SEED codes, Bluetooth PIN and calibration signals.
4. **Power:** Available when used with the Power Pack Module described in section 2.4.4
5. **Trigger:** Enables setup of triggers to generate events when predefined thresholds are breached.
6. **Data Stream:** Provides options to configure channels to stream.
7. **Data Record:** Provides options to configure channels that will be recorded to the onboard SD card.
8. **Storage:** Provides access to recorded miniSEED data, as well as metadata and logs.

## 3.4. Station Metadata

In this section we discuss naming conventions, focusing on SEED (Standard for the Exchange of Earthquake Data) names and how to configure them for your station. While the guidance provided here is advisory, it is recommended to establish a consistent naming scheme for your network to support future expansion.

SEED names are standardized identifiers used in seismology to uniquely label stations, networks, and channels. They consist of a network code, station code, location code, and channel code, allowing instruments and data streams to be easily recognised and analysed. You can read more about SEED names on Earthscope website: [SEED Channel Names](#)

To configure your station names, login as either user or administrator and navigate to the **Setup** tab. Under the heading "Station Config" you will find several fields that define your

station's identity and how it is represented both in the interface and in SEED-formatted data. Some fields are used for SEED naming, while others are for display purposes in Discovery and the web interface:

Digitiser Config					
Auto Refresh	<input type="text" value="1"/>	Auto Reboot	<input type="text" value="On Error"/>	Filter quality	<input type="text" value="High"/>
Station Config					
Host Label	<input type="text" value="Artius_200Hz"/>	Station Code	<input type="text" value="06CF6"/>	Network Code	<input type="text" value="DG"/>
SeedLink SOH Location Code	<input type="text" value="00"/>			Site Name	<input type="text" value="No site"/>

Field	Description	SEED-related
Host Label	A user-friendly name for the instrument in the web interface and Discovery.	No
Station Code	The station code used to identify this station, forming the second part of a SEED name.	Yes
Network Code	A two-character identifier for the network this station belongs to, forming the first part of a SEED name.	Yes
Site Name	A descriptive name for the station location in Discovery.	No
SeedLink SOH Location Code	The SEED location code used for text-based status messages in SeedLink.	Yes

## 3.5. Timing Options

The Artius system synchronises its sample clock using an integrated GNSS receiver.

The currently supported GNSS systems are Navstar (GPS), GLONASS, BeiDou and Galileo.



**Note:** The GNSS can use only three different types of satellites simultaneously and GPS is always used, if available. The other two spots available can be either GLONASS, BeiDou or Galileo.

If visibility of the satellite constellation is available, this is the most accurate way to synchronise your Artius.

### 3.5.1. GNSS lock status

This is available in the **Status** tab of the instrument's web page.

GNSS Status			
GNSS connection status	Connected	Last timestamp	2026-01-27 14:08:36
Last lock time	2026-01-27 14:02:50	GNSS stability	100%
Latitude	51.36077	Longitude	-1.1635
Altitude	125.1	Horizontal dilution of precision	1.13
GNSS PPS status	Trusted Pulsing	GNSS NMEA stream	Input OK
GNSS Lock state	3D locked	Number of satellites	Used: 12 In view: 1



A number of GNSS reporting parameters are given, including:

- Connection status

- Last GNSS update (sync) & last GNSS lock date/time
- GNSS Stability:
  - 0% = no receiver connected.
  - 1% = receiver connected, but waking up (this can occur if the GNSS receiver has been moved a long distance since last power-up).
  - 2-99% = view of sky obstructed.
  - 100% = normal operation with clear view of sky
- Latitude, longitude, altitude
- Horizontal dilution of precision (quality of satellite fix due to position of satellites relative to receiver)
- GNSS PPS status
- GNSS NMEA streaming
- GNSS lock state (No lock/2D/3D)
- Number of available satellites (in use / in view)

### 3.5.2. NTP (Network Timing Protocol) configuration

This gives the system time to within 1 second. It is not generally recommended that this is used as the main time source for deployments. GNSS offers accurate time for this purpose.

By default, the NTP server option (located under the **Network** tab of the instrument's web page) is set to "Pool" which uses the virtual server pool `pool.ntp.org`. This accesses a dynamic collection of networked computers that voluntarily provide moderately accurate time via the NTP to clients worldwide.

Alternatively, it is possible to specify the IP address of your preferred NTP server. To do this, select the "Static" option from the "NTP server" drop-down menu, which activates the "NTP IP Addr" setting, and enter the IP address of your NTP server here.

Network Timing					
Lock to	NTP	NTP Mode	Static	NTP Lock	100
			Server	Registry	
Registry Update	Every 10 secs	Group ID	Pool	Registry Address	52.34.40.123
Registry Address	0.0.0.0	Registry Address	Static	Registry Address	0.0.0.0

### 3.6. Data Transmission

The monitoring and configuration of transmitted data is handled using the **Data Stream** tab of the instrument's webpage.



System type: Artius | Host label: Artius\_200Hz | Host name: ART-6CF6 (10.20.0.22) | Serial number: 06CF6

Data Stream			
<input type="button" value="Disable All Streams"/>	<input type="button" value="Restore default"/>	The "Disable All" and "Restore default" button will ALSO affect settings of any other sensors	<input type="button" value="Reboot"/>
<input type="button" value="Copy to Data Record"/>	"Copy to Data Record" will apply settings from this page to recording configuration of all of the sensors.		Total Samples per Second <b>2346</b> GDI Throughput (kbps) <b>Undefined</b>
Display Streams <input type="button" value="Enabled Only"/>	<input checked="" type="checkbox"/> Apply configuration for tap groups		Display On Page <input type="button" value="Sensor 0"/>
Channels configuration			
Channel sampling rate	Data transform	SEED name - please use check-box to modify the default	RESPonse file - if available
Seismic channels			
InstZ_0 500 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .CHZ	<a href="#">RESP file 5</a>
InstZ_1 5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MHZ	<a href="#">RESP file 6</a>
InstN_0 500 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .CHN	<a href="#">RESP file 8</a>
InstN_1 5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MHN	<a href="#">RESP file 9</a>
InstE_0 500 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .CHE	<a href="#">RESP file 11</a>
InstE_1 5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MHE	<a href="#">RESP file 12</a>
Mass position channels			
MassZ_0 5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MMZ	<a href="#">RESP file 16</a>
MassN_0 5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MMN	<a href="#">RESP file 18</a>
MassE_0 5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MME	<a href="#">RESP file 20</a>
MEMS accelerometer channels			
AccelZ_ 10 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .BNZ	<a href="#">RESP file 38</a>
AccelN_ 10 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .BNN	<a href="#">RESP file 40</a>
AccelE_ 10 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .BNE	<a href="#">RESP file 42</a>
Auxiliary channels			

A brief description of each channel is available by hovering the mouse cursor on the channel name.



**Note:** When changing a setting in the Artius webpage, ensure that you wait until the page refreshes before changing another setting. This allows time for the previous change to take effect.

The drop-down box named **Display Streams** found within the Data Stream section of the page filters out visible channels with options for All, Enabled Only and Disabled Only.

The option **Apply configuration for tap groups** automatically applies the same configuration to the three streams that belong to the same tap (e.g. InstZ\_0, InstN\_0, InstE\_0).

The Channel configuration section is divided into four columns:

- In the first column "Channel sampling rate", drop-down boxes are available for each channel to either select a sample rate or to exclude the channel from streaming by selecting the Disabled option (under the lowest sample rate available). All channels can be stopped from being streamed by clicking the **Disable All** button. The same configuration can be applied to recorded channels by clicking the **Copy to Data Record** button. The default channel configuration can be applied by clicking the **Restore default** button.
- Contrary to the Minimus digitiser, transforms are not supported by Minimus Lite and therefore Artius, and this is reflected in the second column "Data transform".

- In third column “SEED name”, Location and Channel SEED codes can be configured. Options are greyed out with default values applied; they can be edited by clicking on the checkbox at the start of the cell.
- In fourth column “RESPonse file” there are links to the RESP files associated to each of the seismic channels (see Section 4.2.1 more details).

All streaming can be stopped by clicking the **Disable All Streams** button. The same configuration can be applied to recorded channels by clicking the **Copy to Data Record** button. Default channel configuration can be applied by clicking the **Restore Default** button.

Upon changing the sample rate, enabling a transform, or changing Location and Channel codes, the Minimus will need to be restarted for the changes to come into effect; this can be done by pressing the **Reboot** button. During the reboot, the LEDs will flash, displaying the starting-up sequence (see Section 2.3.4) and you will momentarily lose connection to the webpage.

Once the Artius has successfully rebooted, the full web browser display and controls will be available for use.

## 3.7. Data Recording

The main panel of the **Data Record** tab in the web interface is shown here:

Data Record			
<b>Disable All</b>	<b>Restore default</b>	The “Disable All” and “Restore default” button will ALSO affect settings of any other sensors	<b>Reboot</b>
<b>Copy to Data Stream</b>	“Copy to Data Stream” will apply settings from this page to streaming configuration of all of the sensors.		Recording status <b>Recording</b>
Display Streams <b>Enabled Only</b>	<input checked="" type="checkbox"/> <b>Apply configuration for tap groups</b>		For more information about microSD cards status please visit “Storage” tab
<b>Channels configuration</b>			
Channel sampling rate	Data transform	SEED name - please use check-box to modify the default	RESPonse file - if available
<b>DInstrument Seismic channels</b>			
InstZ_sd	500 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .CHZ <a href="#">RESP file 7</a>
InstN_sd	500 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .CHN <a href="#">RESP file 10</a>
InstE_sd	500 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .CHE <a href="#">RESP file 13</a>
<b>DInstrument Mass position channels</b>			
MassZ_sd	5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MMZ <a href="#">RESP file 17</a>
MassN_sd	5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MMN <a href="#">RESP file 19</a>
MassE_sd	5 Hz	Transforms not available on Minimus2	<input type="checkbox"/> DG.06CF6.1 .MME <a href="#">RESP file 21</a>

A brief description of each channel is available by hovering the mouse cursor on the channel name.



**Note:** When changing a setting in the Artius webpage, ensure that you wait until the page refreshes before changing another setting. This allows time for the previous change to take effect.

The drop-down box named **Display Streams** found within the Data Stream section of the page filters out visible channels with options for All, Enabled Only and Disabled Only.

The option **Apply configuration for tap groups** automatically applies the same configuration to the three streams that belong to the same tap (*e.g.* InstZ\_sd, InstN\_sd, InstE\_sd).

The page is divided in four columns:

- In the left-most column, drop-down boxes are available for each channel to either select a sample rate or to exclude the channel from streaming (by selecting the “Disabled” option). All streaming can be stopped by clicking the

**Disable All** button. The same configuration can be applied to real-time transmission channels by clicking the **Copy to Data Stream** button. The default channel configuration can be applied by clicking the **Restore default** button.

- Contrary to the Minimus digitiser, transforms are not supported by Minimus Lite and therefore Artius, and this is reflected in the second column “Data transform”.
- In third column from left, Location and Channel SEED codes can be configured. Cells are greyed out by default (default values applied) and they can be edited by clicking on the check-box.
- In most-right column contains links to the RESP files associated to each of the seismic channels (see Section 4.2.1).

Upon changing the sample rate, or changing Location and Channels codes, the Artius needs to be restarted for the changes to come into effect; this can be done by pressing the **Reboot** button. During the reboot, the LEDs will flash, displaying the starting-up sequence (see Section 2.3.4) and you will momentarily lose connection to the webpage.

Once the Artius has successfully restarted, the full web browser display and controls will be available for use again.

## 3.8. Earthquake Early Warning

The **Trigger** tab is dedicated to Earthquake Early Warning settings. These are disabled by default because of the amount of processing resource – and hence, power – consumed by triggering calculations.

### 3.8.1. Trigger Configuration

The Trigger Configuration section of the web page under the **Triggers** tab enables the user to configure the triggering system. The trigger taps should first be selected from the drop-down list of all possible channels.

Trigger Configuration	
Tap Trigger A	Channel <input type="text" value="None"/>
Tap Trigger B	Select the channel you wish to activate a trigger on.

The heart of the Earthquake Early Warning subsystem are the triggering algorithms: an STA/LTA (Short-Time-Average divided by Long-Time-Average) and Threshold (level) algorithms.

#### 3.8.1.1. Common options

**Channel** - Once this is selected, options will appear to enable the sending of a CAP message, configure the sample rate the trigger will use, select the trigger type, and all the necessary triggering options required.

**Trigger SPS** - It is recommended that Trigger SPS is kept the same as the channel it is on. I.e., if InstZ is streaming at 250 sps, then Trigger SPS should be set to 250 sps to perform the best STA/LTA calculations.

**Trigger Type** – STA/LTA or Threshold

**CAP Enabled** – This option will allow the sending of a CAP message on the initial trigger, when enabled it will also show the option for Peak Window which is a time after the initial trigger in which Peak Ground data will be measured. If the Peak Window is set to a number other than 0, a second CAP message will be sent after the window expires containing the peak value measured.

**Timeout** – After an event has occurred, subsequent triggers within this window will be treated as part of the same event (while also restarting the timeout period).

### 3.8.1.2. STA/LTA

Trigger Configuration			
Tap Trigger A	Channel <input type="text" value="InstZ"/>	Trigger SPS <input type="text" value="50 Hz"/>	Trigger Type <input type="text" value="STA/LTA"/>
Cap Enabled <input type="text" value="yes"/>	Timeout (Seconds) <input type="text" value="10"/>	Detrigger Threshold <input type="text" value="6"/>	Trigger Threshold <input type="text" value="8"/>
Peak Window (Seconds) <input type="text" value="3"/>	STA Period (Seconds) <input type="text" value="1"/>	LTA Period (Seconds) <input type="text" value="60"/>	DC Frequency (Hz) <input type="text" value="0"/>
A window of time after the initial trigger used to capture the Peak Ground value.		Channel <input type="text" value="None"/>	

The STA/LTA algorithm continuously calculates the average values of the absolute amplitude of a seismic signal in two simultaneous moving-time windows. The short-time-average (STA) is sensitive to seismic events while the long-time-average (LTA) provides information about the current amplitude of seismic background noise at the site.

**Trigger Threshold** – When the ratio of STA to LTA exceeds the set threshold value an event is “declared”. To trigger below a ratio value instead of above, simply set the detrigger threshold to be higher than the trigger threshold.

**Detrigger Threshold** – This is the ratio value to stop triggering. This will likely happen within the Timeout. The trigger event itself will only end when the Timeout and Detrigger conditions have been met.

**STA Period** – Number of seconds to measure the short period

**LTA Period** – Number of seconds to measure the long period

**DC Frequency** – The cut-off frequency of the high pass filter in Hz

### 3.8.1.3. Threshold

Trigger Configuration			
Tap Trigger A	Channel <input type="text" value="InstZ"/>	Trigger SPS <input type="text" value="50 Hz"/>	Trigger Type <input type="text" value="Threshold"/>
Cap Enabled <input type="text" value="yes"/>	Timeout (Seconds) <input type="text" value="10"/>	Detrigger Threshold <input type="text" value="6"/>	Trigger Threshold <input type="text" value="8"/>
Peak Window (Seconds) <input type="text" value="3"/>			Absolute Mode <input type="text" value="Real"/>
A window of time after the initial trigger used to capture the Peak Ground value.		Channel <input type="text" value="None"/>	

**Trigger Threshold** - The threshold algorithm, instead, declares the presence of an event when the signal exceeds a particular value. To trigger below a value instead of above, simply set the detrigger threshold to be higher than the trigger threshold.

**Detrigger Threshold** - This is the signal value to stop triggering. This will likely happen within the Timeout. The trigger event itself will only end when the Timeout and Detrigger conditions have been met.

**Absolute Mode** – The signal value used to trigger can be Real, Absolute, or Absolute (No DC). The latter is an option for seismic channels to remove the DC offset.

Although the above is available, it is recommended to use STA/LTA for seismic triggers as it was developed specifically to address the pitfalls of threshold triggering.

### 3.8.2. CAP receiver

The EEW Configuration section of the web page under the **Triggers** tab controls the CAP message configuration parameters, which include the IP address and Port No. of the CAP message receiver as well as other configuration parameters for the contents of the CAP message.

Güralp Discovery includes a CAP (Common Alerting Protocol) receiver. It listens on a specified UDP port for incoming CAP messages. When one arrives, it is displayed and plotted on a map. In addition, the receiver can open a TCP connection to the cloud-based registry server and display CAP messages that have been sent to the registry server.




**Note:** For more details about the Discovery's built-in receiver and configuration of the registry server, please see Discovery manual.

### 3.8.3. STA/LTA Streams

After enabling a trigger, a system reboot is required for the changes to take effect. Once the device restarts, additional data streams become available, displaying the calculated STA, LTA and their ratio (STA/LTA)

The STA/LTA ratio is evaluated against a threshold configured as described above. Viewing these streams is recommended to better understand the behaviour of the ratio values and to assess the impact of the selected time windows.

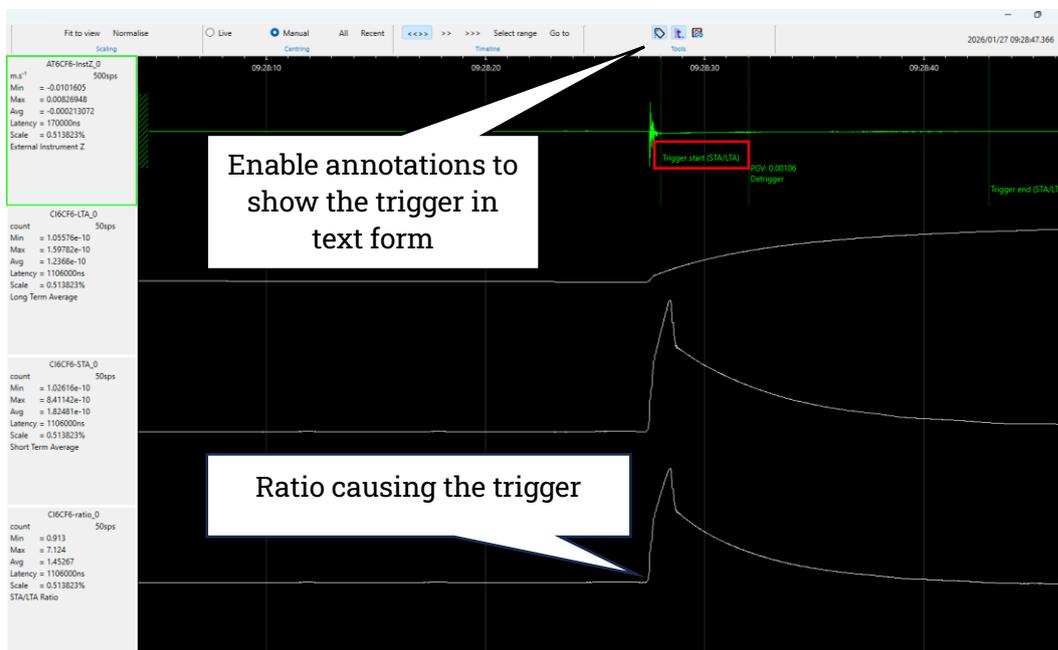

### 3.8.4. Seismic Event Table

The Artius can generate a “Seismic Event Table”. This is list of events detected by the STA/LTA or threshold trigger enabled on taps. It contains information about the time when the event occurred, its duration, the channel that generated the trigger and the peak magnitude of the event. The seismic data before, during and after the event are saved in miniSEED format and can be downloaded using links in the table.

The table is located at the top of the **Trigger** tab in the web page. It might be necessary to refresh the webpage after a trigger is detected to see the even in the Seismic Event Table.

Seismic Events Table			
Download Settings:	Seconds Pre <input type="text" value="10"/>	Seconds Post <input type="text" value="10"/>	<input checked="" type="checkbox"/> Download Z,N,E Triplet
Time of Event Duration	Trigger Function (Tap) Max Signal Diff	Download Source Tap	Download
Tue Jan 27 09:34:00 2026 < 1 second	STA/LTA trigger on channel InstZ (InstZ_tr) N/A	<input type="text" value="InstZ_sd"/>	<a href="#">Request Event Data</a>
Tue Jan 27 09:32:30 2026 < 1 second	STA/LTA trigger on channel InstZ (InstZ_tr) N/A	<input type="text" value="InstZ_sd"/>	<a href="#">Request Event Data</a>
			<input type="button" value="Clear Events"/>

The Artius allows the download of event data in miniSEED format in a time range that is user selectable. The user can select how many seconds before and after the event detection to include in the miniSEED file.

Seismic Events Table			
Download Settings:	<input type="text" value="10"/> Seconds Pre	<input type="text" value="10"/> Seconds Post	<input checked="" type="checkbox"/> Download Z,N,E Triplet

The event table shows which of the components has caused the trigger and the user can choose to either download data related to that single component by deselecting the option "Download Z,N,E Triplet" or download data for all three components by leaving the option enabled.

Seismic Events Table			
Download Settings:	<input type="text" value="10"/> Seconds Pre	<input type="text" value="10"/> Seconds Post	<input checked="" type="checkbox"/> Download Z,N,E Triplet

The last column of the table contains links to downloaded and saved miniSEED files related to each event.

Seismic Events Table			
Download Settings:	Seconds Pre <input type="text" value="10"/>	Seconds Post <input type="text" value="10"/>	<input checked="" type="checkbox"/> Download Z,N,E Triplet
Time of Event Duration	Trigger Function (Tap) Max Signal Diff	Download Source Tap	Download
Tue Jan 27 09:34:00 2026 < 1 second	STA/LTA trigger on channel InstZ (InstZ_tr) N/A	<input type="text" value="InstZ_sd"/>	<a href="#">Request Event Data</a>
Tue Jan 27 09:32:30 2026 < 1 second	STA/LTA trigger on channel InstZ (InstZ_tr) N/A	<input type="text" value="InstZ_sd"/>	<a href="#">Request Event Data</a>
			<input type="button" value="Clear Events"/>




**Note:** The links produce downloadable miniSEED files if and only if the requested data is available in the microSD card. This depends on last flushing time and selected post event time. Use the **flush data** button in the Storage tab to copy most recent data into the microSD cards (see Section 4.1.2).

## 4. Data Access

### 4.1. Seismic and SOH miniSEED files

#### 4.1.1. Data download: Discovery's Docking Station Tool

For data handling, including data download, Güralp recommends using the dedicated **Docking Station** tool available in Discovery 2 (version 2.1.3559 onwards): this tool offers a fast and streamlined data download process. The applet is available from the Tools menu of Discovery's main window and looks like in the figure below.

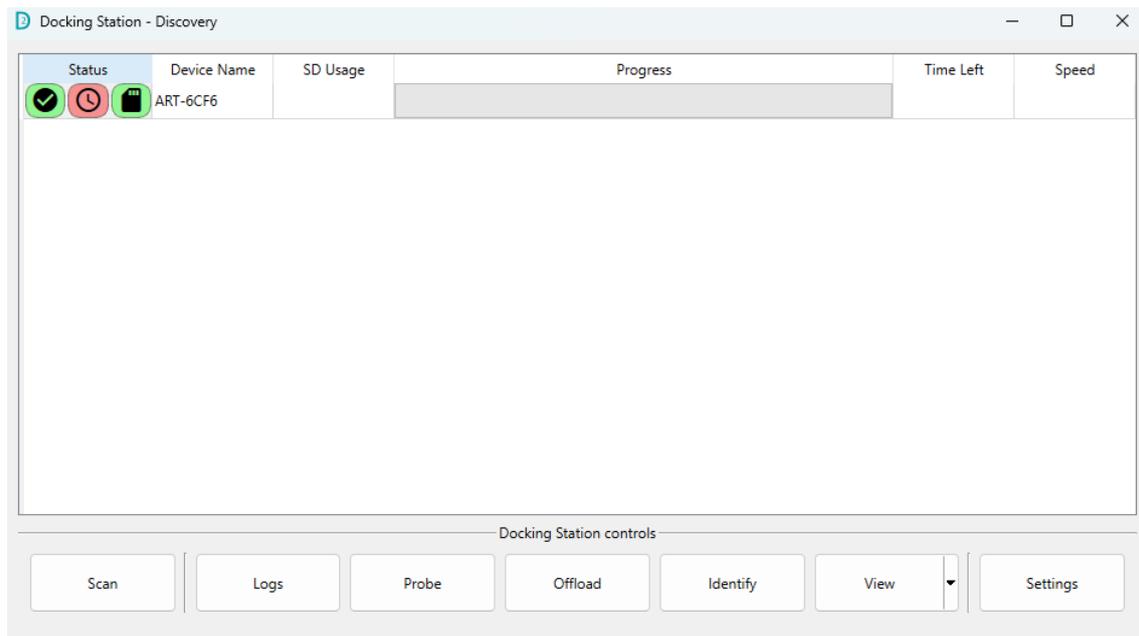

**Note** Please refer to the [Discovery manual](#) (under the "Tools Menu" section) for more details and user instructions.

#### 4.1.2. Bulk Data Download via Webpage

An alternative way to download data from the Artius is through the **Storage** tab of the web interface. This tab displays the miniSEED files stored on the microSD card:



**Artius**

Status Network Setup Power Trigger Data Stream Data Record **Storage** Logout Help

System type: Artius | Host label: Artius\_200Hz | Host name: ART-6CF6 (10.20.0.22) | Serial number: 06CF6

**SD Card control**

Format Progress: 0%

---

**SD Cards status**

Internal microSD card present	PRESENT	External microSD card present	NOT PRESENT
Internal microSD card is recording samples	RECORDING	External microSD card is recording samples	RECORDING
Number of 128-MiB miniSEED files	17	Percentage Free	100
microSD card Internal capacity	60817408 KiB	microSD card External capacity	UNKNOWN

---

**Channel data download by time selection**

Channel:  From:  --:-- To:

---

**SD Card files**

<input type="checkbox"/>	Filename	Size (bytes)	Start data timestamp	Last data timestamp
<input type="checkbox"/>	000_InstE_sd.mseed	53248	2026-01-27 14:18:27	--> 2026-01-27 14:19:12
<input type="checkbox"/>	001_InstN_sd.mseed	49152	2026-01-27 14:18:27	--> 2026-01-27 14:19:12
<input type="checkbox"/>	002_InstE_sd.mseed	57344	2026-01-27 14:18:27	--> 2026-01-27 14:19:12
<input type="checkbox"/>	003_Calibration_sd.mseed	12288	2026-01-27 14:18:27	--> 2026-01-27 14:19:12
<input type="checkbox"/>	004_InstX_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:12
<input type="checkbox"/>	005_MassE_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:10
<input type="checkbox"/>	006_MassN_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:10
<input type="checkbox"/>	007_MassE_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:10
<input type="checkbox"/>	008_Voltage_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	009_Power_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	010_Humidity_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	011_Temperatur_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	012_AccelE_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	013_AccelN_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	014_AccelE_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	015_Phase_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13
<input type="checkbox"/>	016_DAC_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13

---

**Auxiliary files**

Filename	Description
DG_06CF6_dataless	Dataless SEED file
sensor0.xml	Station/XML file
system.log	System log file
status.log	Status log file
calvals.txt	SCREAM! calibration values
poleszero.txt	SCREAM! zeros, poles and gains
calib.txt	Calibration text file
seedlink.log	Seedlink server log
event_table.txt	Table of Events
crashlog.txt	Log of any crashes

Guralp Systems Limited  
 Midas House, Calleva Park, Aldermaston, Reading, RG7 8EA, UK  
 Tel: +44 118 981 9058, Fax: +44 118 981 9943  
 E-Mail: sales@guralp.com, support@guralp.com

Single or multiple files can be downloaded simultaneously by ticking the check-boxes on the left of each link and clicking on **Download Selected Files** button. Pressing **Flush data** is recommended first to force-write the most recent data from the internal buffer to the SD cards.

### 4.1.3. Time-Based Data Download via Webpage

From the **Storage** tab of the web interface, data for a single stream spanning a specific time-interval can be downloaded. To do this, start by selecting the desired stream from the drop-down menu:

Channel data download by time selection				
Channel: DG.06CF6.1.CHZ [InstZ_sd]		From: dd/mm/yyyy	To: dd/mm/yyyy	Download
SD Card files				
File	Size (bytes)	Start data timestamp	Last data timestamp	
<input type="checkbox"/> 000_InstZ_sd.mseed	DG.06CF6.1.CHN [InstN_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:12	
<input type="checkbox"/> 001_InstN_sd.mseed	DG.06CF6.1.CHE [InstE_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:12	
<input type="checkbox"/> 002_InstE_sd.mseed	DG.06CF6.1.HHX [InstX_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:12	
<input type="checkbox"/> 003_Calibration_sd.mseed	DG.06CF6.1.MMZ [MassZ_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:12	
<input type="checkbox"/> 004_InstX_sd.mseed	DG.06CF6.1.MMN [MassN_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:12	
<input type="checkbox"/> 005_MassZ_sd.mseed	DG.06CF6.1.MME [MassE_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:12	
<input type="checkbox"/> 006_MassN_sd.mseed	DG.06CF6.1.CC0 [Calibration_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:10	
<input type="checkbox"/> 007_MassE_sd.mseed	DG.06CF6.1.MQV [Voltage_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:10	
<input type="checkbox"/> 008_Voltage_sd.mseed	DG.06CF6.1.MYP [Power_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:10	
<input type="checkbox"/> 009_Power_sd.mseed	DG.06CF6.1.BIH [Humidity_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	
<input type="checkbox"/> 010_Humidity_sd.mseed	DG.06CF6.1.BKT [Temperatur_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	
<input type="checkbox"/> 011_Temperatur_sd.mseed	DG.06CF6.1.BNZ [AccelZ_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	
<input type="checkbox"/> 012_AccelZ_sd.mseed	DG.06CF6.1.BNN [AccelN_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	
<input type="checkbox"/> 013_AccelN_sd.mseed	DG.06CF6.1.BNE [AccelE_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	
<input type="checkbox"/> 014_AccelE_sd.mseed	DG.06CF6.1.LYP [Phase_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	
<input type="checkbox"/> 015_Phase_sd.mseed	DG.06CF6.1.LYD [DAC_sd]	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	
<input type="checkbox"/> 016_DAC_sd.mseed	8192	2026-01-27 14:18:27	--> 2026-01-27 14:19:13	

Next select the start and end dates using the pop-up calendar, then the desired time range in 24-hour format :

Channel data download by time selection										
Channel: DG.06CF6.1.CHZ [InstZ_sd]		From: dd/mm/yyyy	To: dd/mm/yyyy	Download						
		January 2026	↑ ↓							
File	Size (bytes)	Mo	Tu	We	Th	Fr	Sa	Su	stamp	Last data timestamp
<input type="checkbox"/> 000_InstZ_sd.mseed	53248									--> 2026-01-27 14:19:12
<input type="checkbox"/> 001_InstN_sd.mseed	49152	29	30	31	1	2	3	4		--> 2026-01-27 14:19:12
<input type="checkbox"/> 002_InstE_sd.mseed	57344	5	6	7	8	9	10	11		--> 2026-01-27 14:19:12
<input type="checkbox"/> 003_Calibration_sd.mseed	12288	12	13	14	15	16	17	18		--> 2026-01-27 14:19:12
<input type="checkbox"/> 004_InstX_sd.mseed	8192	19	20	21	22	23	24	25		--> 2026-01-27 14:19:10
<input type="checkbox"/> 005_MassZ_sd.mseed	8192	26	27	28	29	30	31	1		--> 2026-01-27 14:19:10
<input type="checkbox"/> 006_MassN_sd.mseed	8192	2	3	4	5	6	7	8		--> 2026-01-27 14:19:10
<input type="checkbox"/> 007_MassE_sd.mseed	8192									--> 2026-01-27 14:19:10
<input type="checkbox"/> 008_Voltage_sd.mseed	8192									--> 2026-01-27 14:19:13
<input type="checkbox"/> 009_Power_sd.mseed	8192									--> 2026-01-27 14:19:13
		Clear			Today					

Lastly, click the **Download** button to initiate a file transfer to your local device.

#### 4.1.4. Bulk Data Extraction via Network

Files stored on the SD card can be downloaded using HTTP. The example bash script below can be used from a Linux PC or from the WSL shell on a Windows PC. The script extracts all files from the SD Card into a directory named after the date and the network address of the Artius.

```
#!/bin/bash
# Invoke with one argument: the network
# address of the Minimus

set -x

if [ "$#" -ne 1 ] ; then
    echo "Usage: $(basename $0) network_address"
    exit 1
fi

NET_ADDRESS=$1
DATE=$(date --iso-8601)
SAVEDIR = ${DATE}_${NET_ADDRESS}
echo Saving to $$SAVEDIR

mkdir $$SAVEDIR
```

```
cd $SAVEDIR
wget -rnp http://$NET_ADDRESS/tab9.html
cd ..

echo Done
```

#### 4.1.5. Time Based-Data Extraction via Network

The example Python script below will extract seismic data from the SD card based on a specified time interval. This is similar to the FDSN (International Federation of Digital Seismograph Networks) data archive retrieval service:

<https://www.fdsn.org/webservices/fdsnws-dataselect-1.1.pdf>.

Channel names are as given on the **Data Record** tab of the web interface, and the times are specified in UTC time format. The resulting file will be in miniSEED format.



**Note** The script forms an http request to the instrument in the form of:

```
http://<<IP Address>>/data?channel=<<Channel>>&from=<<Unix Epoch Seconds>>&to=<<Unix Epoch Seconds>>
```

which for the example below, would appear as:

```
http://192.168.254.101/data?channel=DG.TEST.01.CHZ&from=1740114000.0&to=1740117600.0
```

```
import os
import wget
from obspy import read, read_inventory, UTCDateTime
from obspy.signal import PPSD

##### Start of variable to set #####
sensor = "192.168.254.101"
channel = "DG.TEST.01.CNZ"
start = UTCDateTime("2025-02-21T05:00:00.0")
end = UTCDateTime("2025-02-21T06:00:00.0")
##### End of variables to set #####

startUNIX = UTCDateTime(start).timestamp
#We use the 'start'&'end' to cut the data using Obspy
endUNIX = UTCDateTime(end).timestamp
# We use the 'startUNIX'&'endUNIX' to pull the
# data from the Minimus

#if os.path.exists(r"{0}\tt.mseed".format(temp)):
# See if temp file exists, if so delete.
#os.remove(r"{0}\tt.mseed".format(temp))

if os.path.exists(r"{0}_{1}_{2}.mseed".format(sensor, channel,
start)):
    os.remove(r"{0}_{1}_{2}.mseed".format(sensor, channel,
start))

print(start)

print(r"http://{0}/data?channel={1}&from={2}&to={3}".format(sensor,
channel, startUNIX, endUNIX))
```

```
wget.download(r"http://{0}/data?channel={1}&from={2}&to={3}".format(
    sensor, channel, startUNIX, endUNIX),
    r"{0}_{1}.mseed".format(channel, startUNIX))
```

The following example in Bash allows you to extract from the SD card the three seismic components of a sensor for a given date over a specified time frame. It then combines the three components into an individual miniSEED file, whose name will include the network code, station code, start date and start time:

```
#!/bin/bash
# Invoke with one argument: the IP address. For example
./script_name 192.168.254.101

set -x

# enter your network details
net_code=DG
station_code=04D67
location_code=0L

#enter the sensor codes for the location targeted, found on the
Data Stream tab of discovery, the last 3 characters/values of the
SEED name (HNZ)
sensor_code1=HNZ
sensor_code2=HNN
sensor_code3=HNE

# choose the day
day=2024-04-28

# choose the start time in 24-hour format (e.g. 16 = 4pm)
start_hour=16

# choose the number of hours to include in the miniSEED file(e.g.
1 = 1-hour-long miniSEED)
step=1

utc=$(date --date ${day} +%s)
start_utc=$(expr $utc + 3600 \* ${start_hour})
end_utc=$(expr ${start_utc} + 3600 \* ${step})

echo $utc
echo $start_utc
echo $end_utc

wget -v -Oz_component.mseed
http://$1/data?channel=${net_code}.${station_code}.${location_code}
.${sensor_code1}\&from=${start_utc}\&to=${end_utc}
wget -v -On_component.mseed
http://$1/data?channel=${net_code}.${station_code}.${location_code}
.${sensor_code2}\&from=${start_utc}\&to=${end_utc}
wget -v -Oe_component.mseed
http://$1/data?channel=${net_code}.${station_code}.${location_code}
.${sensor_code3}\&from=${start_utc}\&to=${end_utc}

# Convert from Unix timestamp to date and time
date_string=`date -d @${start_utc} +%Y.%m.%d-%H.%M.%S`

# In this example, the 3-components miniSEED file will be named
"DG.04D67-2024.04.28-16.00.00.mseed"
```

```
cat z_component.mseed n_component.mseed e_component.mseed >
${net_code}.${station_code}-${date_string}.mseed
```

## 4.2. Metadata

The Artius provides several forms of metadata describing the configuration, sensitivity, and response of all connected sensors and digitiser channels. Metadata is essential for understanding and correctly interpreting recorded data. It defines how the digitiser converts analogue motion into digital counts, and how each sensor channel responds across frequency.


The device automatically generates three metadata formats: RESP files, Station XML files, and a Dataless SEED volume. Each format serves a different purpose, ranging from per-channel response information to complete system-wide metadata. The following sections describe each type and explain how to download them.

### 4.2.1. RESPonse Files

RESP files contain channel-specific response information. Each RESP file describes a single sensor channel. This includes the overall sensitivity, gain and filter stages, poles and zeros, and instrument identifiers. They are human-readable text files commonly used by analysis tools such as ObsPy, SAC, and PDCC.

#### Accessing RESP files:

Each channel's RESP file is available from the [Data Stream](#) and [Data Record](#) pages via the RESP file link:

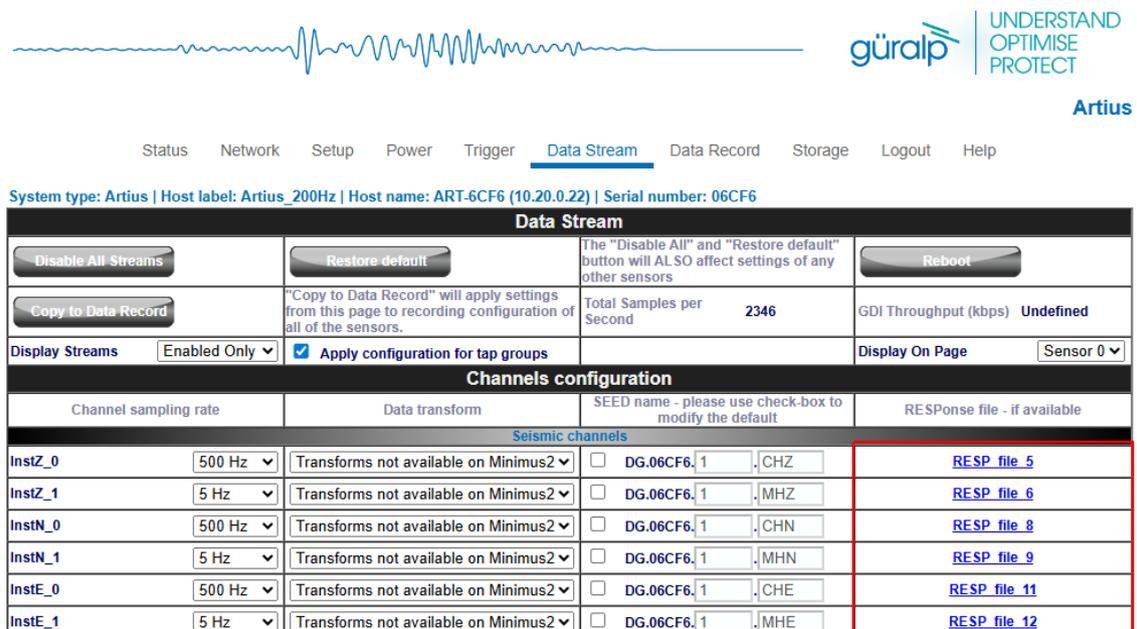

güralp | UNDERSTAND  
OPTIMISE  
PROTECT

Artius

Status Network Setup Power Trigger Data Stream Data Record Storage Logout Help

System type: Artius | Host label: Artius\_200Hz | Host name: ART-6CF6 (10.20.0.22) | Serial number: 06CF6

Data Stream			
<a href="#">Disable All Streams</a>	<a href="#">Restore default</a>	The "Disable All" and "Restore default" button will ALSO affect settings of any other sensors	<a href="#">Reboot</a>
<a href="#">Copy to Data Record</a>	"Copy to Data Record" will apply settings from this page to recording configuration of all of the sensors.	Total Samples per Second <b>2346</b>	GDI Throughput (kbps) <b>Undefined</b>
Display Streams <a href="#">Enabled Only</a>	<input checked="" type="checkbox"/> <a href="#">Apply configuration for tap groups</a>		Display On Page <a href="#">Sensor 0</a>
Channels configuration			
Channel sampling rate	Data transform	SEED name - please use check-box to modify the default	RESP file - if available
<b>Seismic channels</b>			
InstZ_0 <a href="#">500 Hz</a>	<a href="#">Transforms not available on Minimus2</a>	<input type="checkbox"/> DG.06CF6,1, .CHZ	<a href="#">RESP file 5</a>
InstZ_1 <a href="#">5 Hz</a>	<a href="#">Transforms not available on Minimus2</a>	<input type="checkbox"/> DG.06CF6,1, .MHZ	<a href="#">RESP file 6</a>
InstN_0 <a href="#">500 Hz</a>	<a href="#">Transforms not available on Minimus2</a>	<input type="checkbox"/> DG.06CF6,1, .CHN	<a href="#">RESP file 8</a>
InstN_1 <a href="#">5 Hz</a>	<a href="#">Transforms not available on Minimus2</a>	<input type="checkbox"/> DG.06CF6,1, .MHN	<a href="#">RESP file 9</a>
InstE_0 <a href="#">500 Hz</a>	<a href="#">Transforms not available on Minimus2</a>	<input type="checkbox"/> DG.06CF6,1, .CHE	<a href="#">RESP file 11</a>
InstE_1 <a href="#">5 Hz</a>	<a href="#">Transforms not available on Minimus2</a>	<input type="checkbox"/> DG.06CF6,1, .MHE	<a href="#">RESP file 12</a>


Clicking the link opens the RESP information in your browser:

```

#          << Guralp SEED response file builder v2.1-2776 >>
#
#          ===== CHANNEL RESPONSE DATA =====
B050F03  Station:      06CF6
B050F16  Network:       DG
B052F03  Location:       1
B052F04  Channel:       CHZ
B052F22  Start date:    2025,268,15:58:35
B052F23  End date:      No Ending Time
#          =====
#          +-----+-----+-----+-----+
#          +          | Channel Sensitivity, 06CF6 ch CHZ |          +
#          +-----+-----+-----+-----+
#
B058F03  Stage sequence number:      0
B058F04  Sensitivity:                8.196721E+08
B058F05  Frequency of sensitivity:  1.000000E+00 HZ
B058F06  Number of calibrations:    0
#
#          +-----+-----+-----+-----+
#          +          | Response (Poles & Zeros), 06CF6 ch CHZ |          +
#          +-----+-----+-----+-----+
#
B053F03  Transfer function type:      A [Laplace Transform (Rad/sec)]
B053F04  Stage sequence number:      1
B053F05  Response in units lookup:    M/S - Velocity in Metres Per Second
B053F06  Response out units lookup:     V - Volts
B053F07  A0 normalization factor:      1.547554E+06
B053F08  Normalization frequency:     1.000000E+00

```

To download the file, right-click the link and select **Save Link As**:

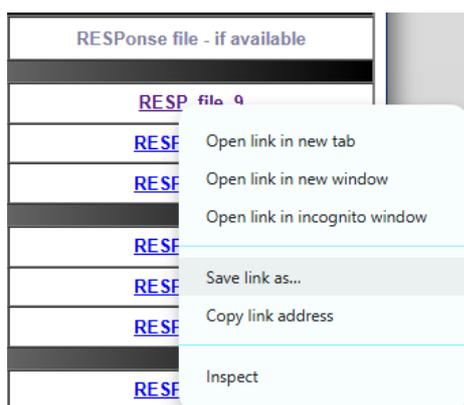

RESP files can also be accessed by URL, for example:

[http://<device-ip>/RESP\\_file\\_<n>.txt](http://<device-ip>/RESP_file_<n>.txt)

Example using wget from a command line:

```
wget http://10.20.1.82/RESP_file_7.txt
```

## 4.2.2. Station XML Files

Station XML is a modern format widely used for exchanging seismic metadata. It contains structured metadata for an entire sensor, including all channel responses, sensor orientation and location, calibration constants, digitiser sensitivity, and station identifiers.

### Accessing Station XML files:

The Station XML file is available from the **Storage** page as Sensor0.xml under the Auxiliary Files.

Auxiliary files	
Filename	Description
DG 06CF6.dataless	Dataless SEED file
sensor0.xml	StationXML file
system.log	System log file
status.log	Status log file
calvals.txt	SCREAM! calibration values
polezero.txt	SCREAM! zeros, poles and gains
calib.txt	Calibration text file
seedlink.log	Seedlink server log
event_table.txt	Table of Events
crashlog.txt	Log of any crashes

They can also be accessed via direct URL, for example:

<http://<device-ip>/sd/Sensor0.xml>

Example using wget from the command line:

```
wget http://10.20.1.82/sd/Sensor0.xml
```

### 4.2.3. Dataless SEED Volume

A Dataless SEED Volume contains all metadata for the digitiser and every connected sensor, including response stages, sensitivities, channel naming, and network/station codes. It does not contain waveform data; instead, it complements miniSEED files by providing the metadata needed to interpret them.

#### Accessing dataless SEED Volume:

The dataless volume is available from the **Storage** page under Auxiliary Files. Clicking the filename will download it directly to your computer:

Auxiliary files	
Filename	Description
DG 06CF6.dataless	Dataless SEED file
sensor0.xml	StationXML file
system.log	System log file
status.log	Status log file
calvals.txt	SCREAM! calibration values
polezero.txt	SCREAM! zeros, poles and gains
calib.txt	Calibration text file
seedlink.log	Seedlink server log
event_table.txt	Table of Events
crashlog.txt	Log of any crashes

It can also be retrieved by URL. The filename is formed from the two-character network code and the station code. For example, if the network code is DG and the station code is TADL, the dataless filename is:

DG\_TADL.dataless

The direct URL would be:

[http://<device-ip>/<net\\_code>\\_<stat\\_code>.dataless](http://<device-ip>/<net_code>_<stat_code>.dataless)

Example using wget from the command line:

```
wget http://10.20.1.82/DG_TADL.dataless
```

## 5. Bluetooth Connectivity: the GüVü App


The GüVü app provides monitoring and control of nearby Artius units using the Bluetooth protocol. It is available for Android devices.

GüVü can be downloaded from the Google Play store at:

<https://play.google.com/store/apps/details?id=com.guralp.whisper>

### 5.1. Getting Stated

To launch GüVü, follow the steps shown in the figure below:

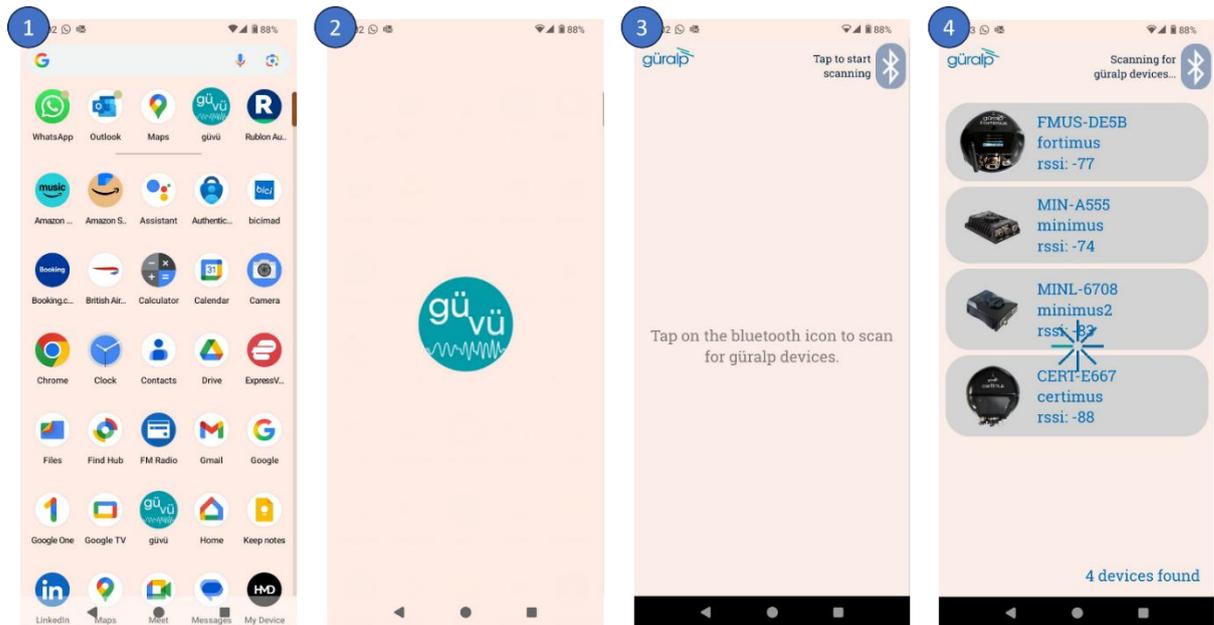


Steps for launching the GüVü App:

1. Launch by clicking on the GüVü icon from either the Apps Menu or from the Home Screen.
2. Wait a few seconds for the app splash screen.
3. Press the Bluetooth icon  to enable Bluetooth connectivity (if not already enabled) and to search for available devices to with which to pair.
4. Select the appropriate device from the list to pair. Wait a few seconds for the main viewer screen to show.

If you experience problems connecting, try going closer to your instrument, or forcing GüVü to quit and then re-launching the app.

Once the device is connected, the main view of the app will be displayed. This screen displays a number of status indicators associated with the Artius.

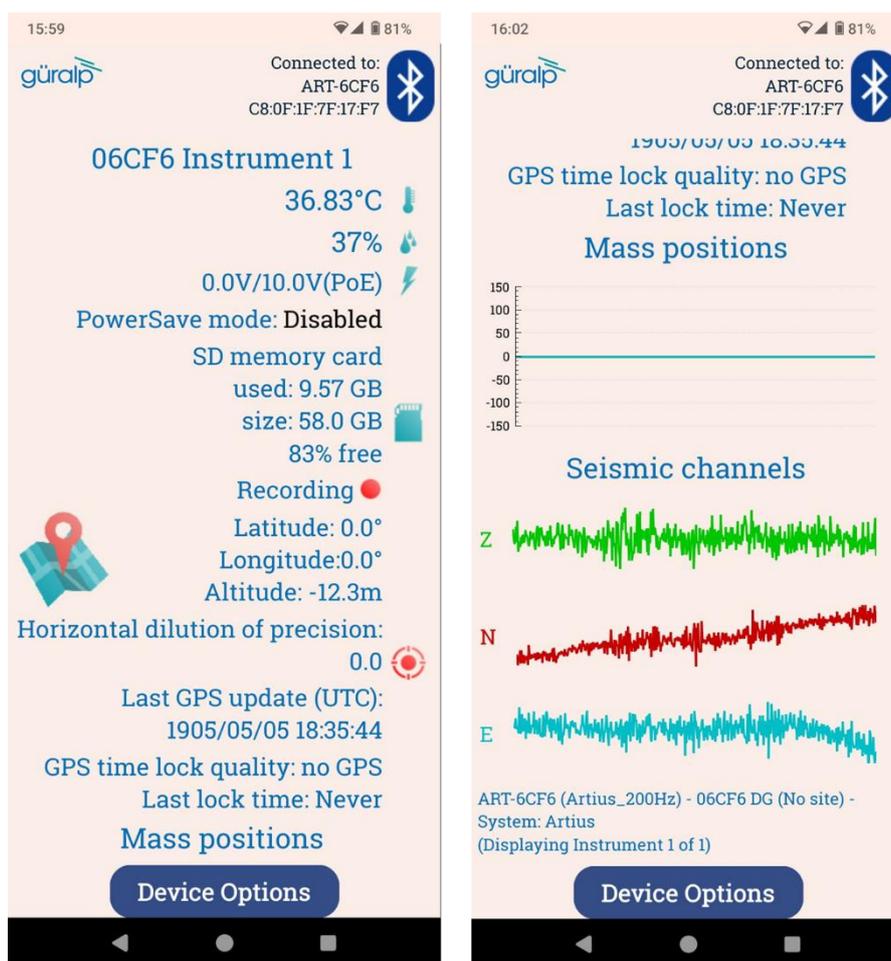

## 5.2. View Settings

The user can customise the view of the main instrument status window. Four different view options can be cycled through by tapping **Device Options** menu on the main instrument status window:

- **Show overview** – the default view setting; show state-of-health status, mass positions, and sensor traces on a single screen.
- **Show status view** – show state-of-health on the main screen only.
- **Show mass graph view** – show mass position traces on the main screen only; and
- **Show velocity graph view** - show sensor traces on the main screen only.

## 5.3. Instrument Control

Several features of the Artius can be controlled and configured remotely over Bluetooth using GüVü:


- Rebooting the Artius
- Station metadata (User Label, Station Name, Network Code, Site Name)
- Network setting (IP, Netmask, Gateway)

- Changing channels' sampling rates

In each case, GüVü will report whether the selected command has been successfully sent to the device.


 **Note:** The GüVü App contains functions for all Güralp instruments, some of which are **not** applicable to the Artius. These include:

- Select data source
- Unlock/Lock sensor mass
- PowerSave modes
- Unmount SD Card

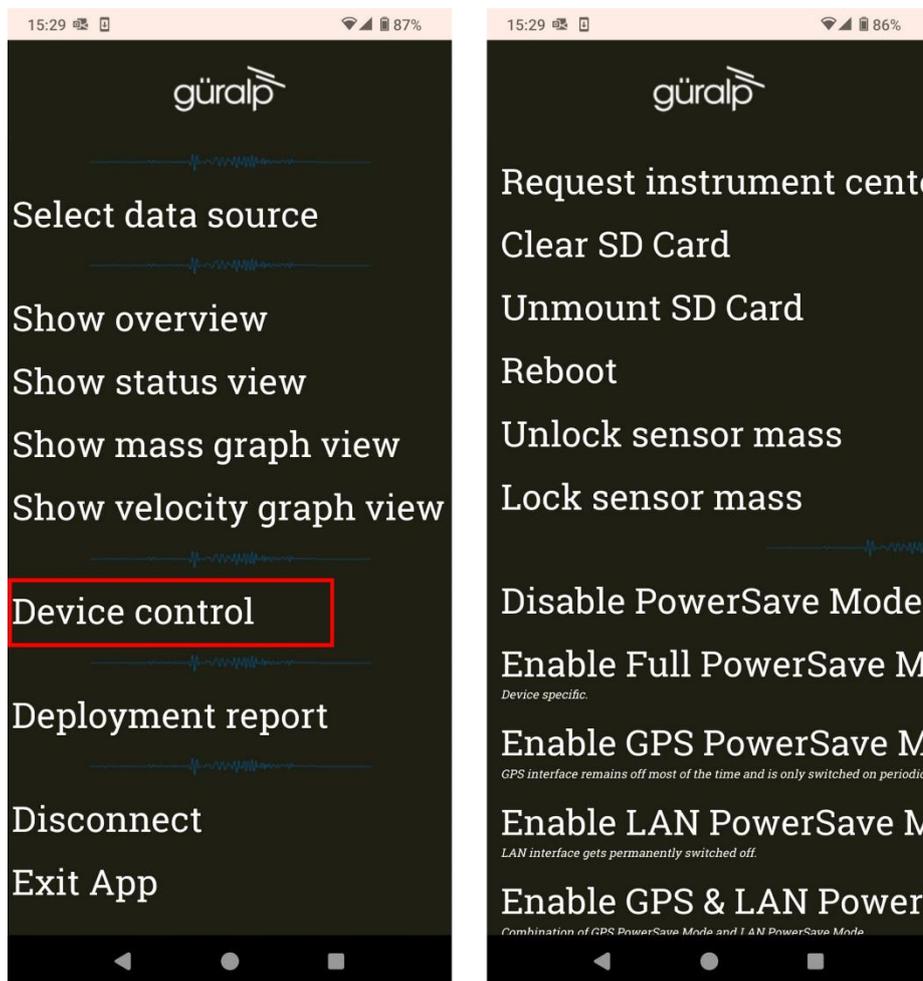

 **Note:** After any modification to channels' sampling rates or network settings (available through "Change station settings") the Artius must be rebooted before the changes will take effect.

These options can be accessed by tapping the **Device Options** menu and choosing the **Device control** option. To access the instrument control and configuration sub-menu, a PIN code has to be entered by selecting the text entry box and tapping **OK**.

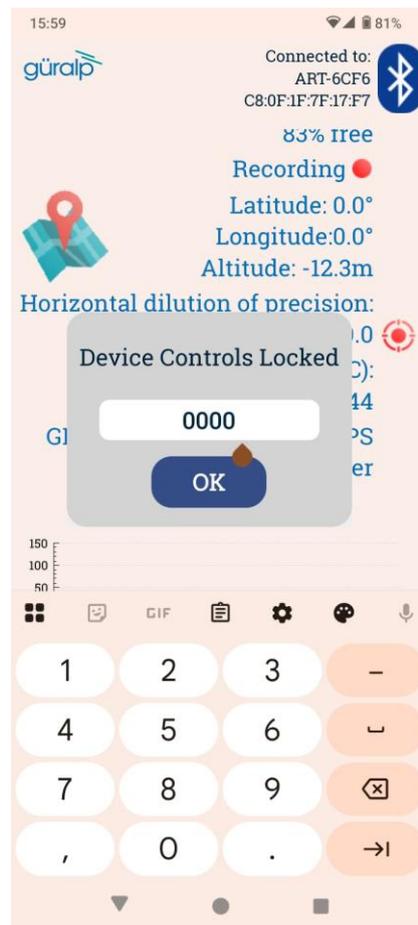


The default PIN code used to access the Instrument Control menu is "0000".



**Caution:** Güralp recommends changing the PIN code from the default, as described in the following section, in order to maintain station security.

### 5.3.1. Setting the PIN Code

The PIN code for accessing the instrument control menu of GüVü can be changed from the Setup tab of the web page. The new four-digit PIN code should be entered into the "Bluetooth PIN" field. The new value is applied by keying Enter; or clicking the left mouse button in any other setting box.



## 5.4. Emailing a Deployment Report

The GüVü app has a feature that allows the user to generate an automatic deployment report that can then be filed via email.

The deployment report includes the following details:

- System name.

- Station name.
- Network code.
- Instrument user label.
- Memory card storage size and recording status.
- Location of site (GNSS latitude, longitude, elevation).
- Time of deployment.
- GNSS lock quality.
- Power supply status.
- Instrument temperature and humidity recordings.

To send a deployment report, tap the **Device Options** menu and choose the "Deployment report" option. GüVü will then open the default email application on the device, showing a draft email which will include the parameters described above.


```
ART-4338 system report
* GENERAL *
Hostname: ART-4338
User label: 16_200Hz
SEED Station name: 04338
SEED Network name: DG
SEED Site name: No site
Digitizer relative humidity: 25%Digitizer
temperature: 39°C
Digital instrument temperature: 0.42°C
Power supply voltage: 0V
Power over ethernet voltage: 11V
Analogue instrument type: Artius
Guralp product name: Artius
* NETWORK *
IP address: 10.30.0.43
Netmask: 255.255.0.0
Default gateway: 0.0.0.0
Mode: Automatic IP (DHCP)
* STORAGE *
Primary microSD card space: 8.78GB/58.0GB
(84%ee)
Primary microSD card status: Recording
Secondary microSD card status: Recording
External microSD: NOT present / NOT usable /
SECONDARY
Internal microSD: Usable / PRIMARY
* GPS *
GPS Quality: 100% Latitude: 51.3612°
Longitude: -1.16422°
Altitude: 111m
Horizontal dilution of precision: 0.5
Time: 2026/01/27 13:39:19
Last lock time: 2026/01/27 09:05:39
* DEPLOYMENT INFO *
```

## 6. Firmware Update

The firmware of the Artius is upgradeable. New releases appear regularly – mostly to add new features but, occasionally, to fix problems. Güralp recommends that the Artius is regularly checked for availability of firmware updates and, when convenient, these updates should be installed. If in doubt whether to upgrade the firmware or not, please check the release notes ([london.guralp.com/download/sw/release\\_ART.shtml](http://london.guralp.com/download/sw/release_ART.shtml)) or contact [support@guralp.com](mailto:support@guralp.com).

To upgrade :


1. Run Discovery.
2. Right-click on the Artius in Discovery main window and select “File Exchange”.
3. In the “File Exchange” tab, click on the Stable or Experimental button depending on which firmware you want to install

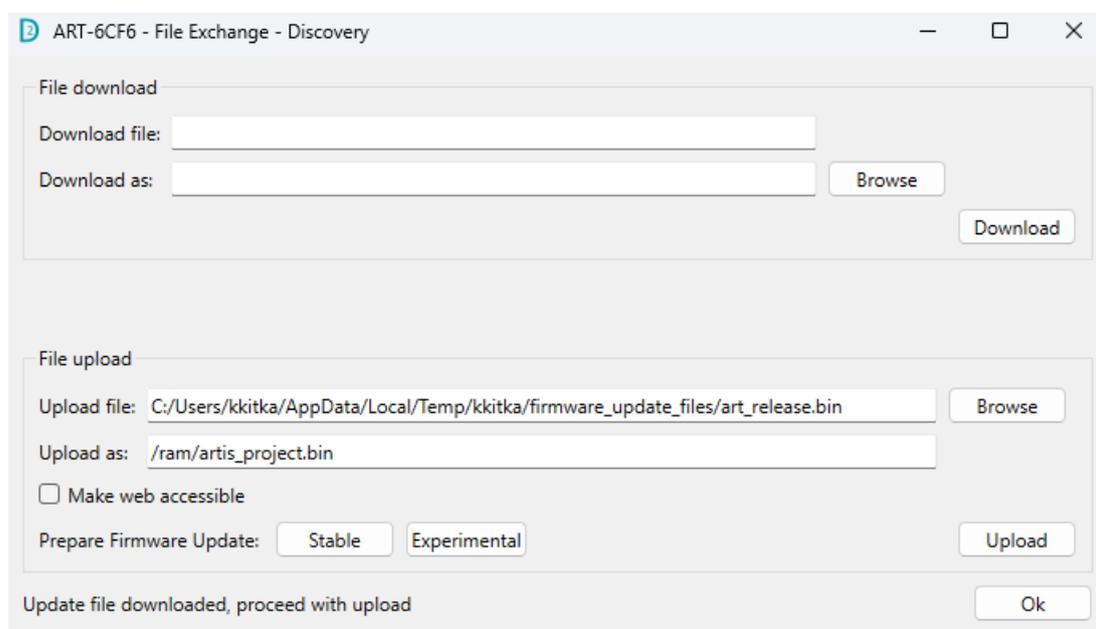

4. Do not change the upload file name but leave it exactly as it automatically appears.
5. Press upload.
6. The upload takes approx. 40 seconds. The LED on the Artius should change colour after the upload completes: persistent red erasing internal FLASH memory, then persistent blue during programming, then finally persistent white when complete.
7. DO NOT remove power for the whole duration of the firmware update



**Note:** IP address, system name, netmask are all preserved. To preserve general settings, offload the config first. Use Discovery, right click and select “System Configuration”. Download first and upload after the update. Uploading will prompt the Artius to reboot automatically.

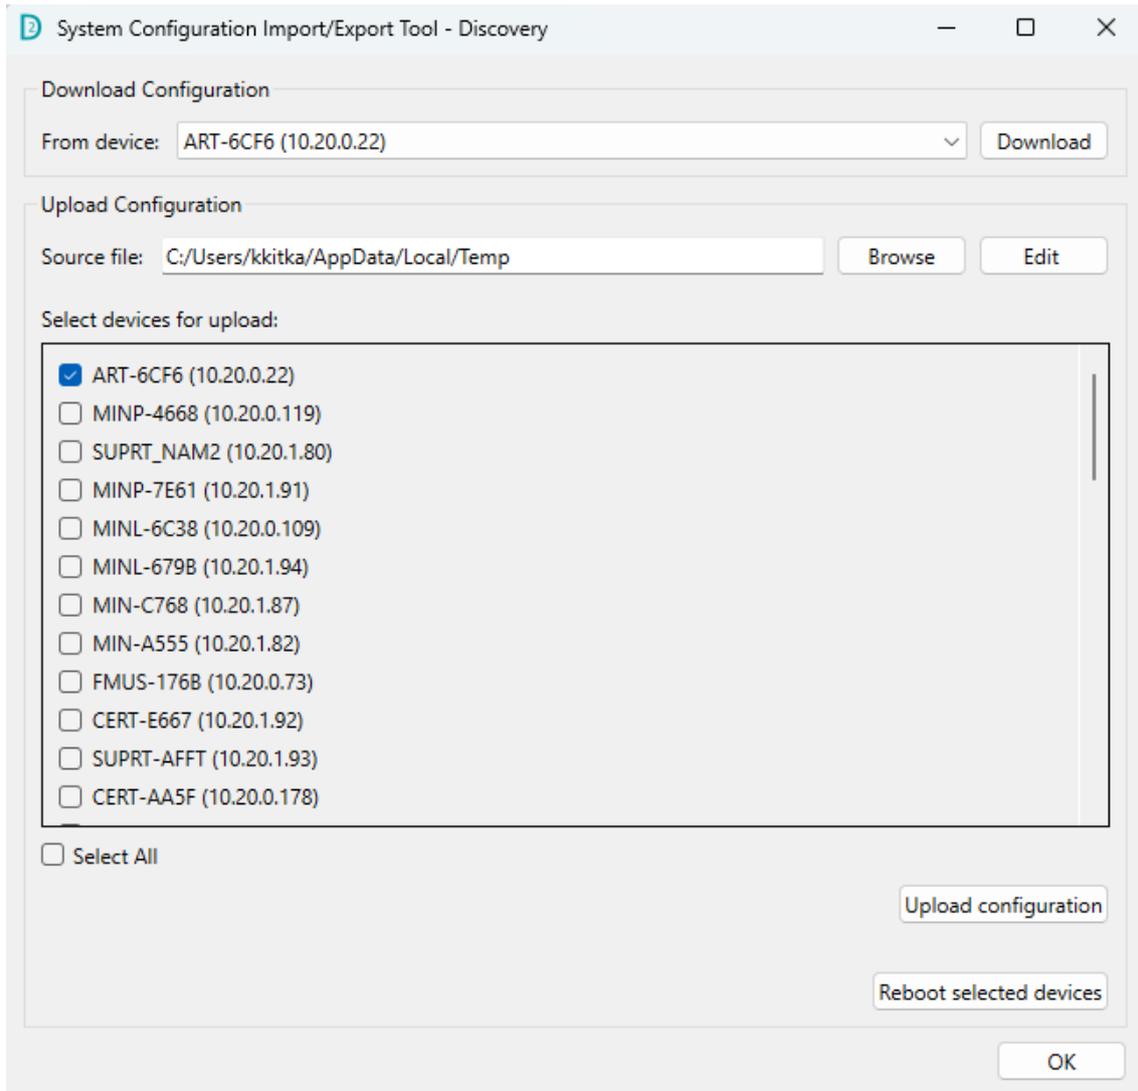

**Caution:** Minimus<sub>2</sub>/Minimus Lite firmware differs from and is incompatible with Artius. Thus, previously saved firmware files for these digitisers should not be uploaded through the File Exchange to the Artius node. The **Stable** and **Experimental** options will automatically pull correct Artius files from the Guralp server. A stable internet connection is advised.

## 7. Installation



**Note:** For further recommendations regarding Artius installation, or if your intended deployment is not covered in this guide, please contact [support@guralp.com](mailto:support@guralp.com).

### 7.1. Direct Burial with PPM

For the best results, Güralp recommends following the installation procedure below.

- **Dig the main hole**

Dig a hole deep enough to reach compact earth. If compacted soil is not accessible, manually compact the base of the hole.

- **Shape the hole**

The hole must have extra space extending southward to accommodate the Artius body and its connector. This orientation ensures that once deployed the Artius points North, with the connector exiting to the South.

- **Set the depth**

The hole should be deep enough so that the top of the Artius sits 1-2 cm above ground level after placement.

- **Prepare the power supply**

Dig a separate hole for the Artius Power Pack Module (PPM) or any compatible 7-16 V DC power source. Dig a connecting trench between the two holes to bury the power cable.

- **Connect the hardware**

Connect the cable to the Artius and attach the spike, if purchased.

- **Place the Artius**

Align the Artius so the North arrow on the device points North. Gently press the spike into the base of the hole, using your foot if necessary.

- **Level the device**

Use the built-in bubble level to check horizontal alignment. If needed, remove and adjust the base of the pit or reposition the Artius using the spike.



- **Lay the cable**  
Ensure the cable is not coiled around the Artius and does not apply any pressure on the connector port. If the cable is too long, coil any excess around the power supply, not the Artius.



- **Connect solar panel (if applicable)**  
Connect solar panels to the Charge Input connector of the PPM before backfilling.

- **Check device status**  
Before the next step, ensure that the Artius LED is flashing three green lights.



- **Backfill and compact**  
Fill both holes and trench with the removed soil or substrate. Compact the surface to minimize future settling.

- **Provide thermal insulation**  
If you expect large thermal variations, insulate the Artius. This can be done by putting some wool sheets or bubble wrap on top of the Artius and covering it with a box.

- **Post-deployment cleanup**  
After retrieving the Artius from the field, remove dirt from the bottom grooves using a stiff nylon brush or similar tool to ensure no mud or dirt is left. Inserting the device into the docking station with dirt might cause damage.

---

## 7.2. Surface Deployment with Spike

- **Connect the hardware**  
Connect the spike to the Artius and find a suitable area with firm soil to place.
- **Place the Artius**  
Align the Artius so the North arrow on the device points North. Gently press the spike into the base of the hole, using your foot if necessary.
- **Prepare the power supply**  
Place the Artius Power Pack Module (PPM) or any compatible 7-16 V DC power source securely to the ground nearby and connect to the Artius.
- **Lay the cable**  
Ensure the cable is not coiled around the Artius and does not apply any pressure on the connector port. If the cable is too long, coil any excess around the power supply, not the Artius. Bury the cable between the power supply and Artius to avoid damage from the environment.

- **Level the device**  
Use the built-in bubble level to check horizontal alignment. If needed, remove and adjust the base of the pit or reposition the Artius using the spike.
- **Connect solar panel (if applicable)**  
Connect solar panels to the Charge Input connector of the PPM.
- **Check device status**  
Before the next step, ensure that the Artius LED is flashing three green lights.
- **Provide thermal insulation**  
If you expect large thermal variations, insulate the Artius. This can be done by putting some wool sheets or bubble wrap on top of the Artius and covering it with a box.
- **Post-deployment cleanup**  
After retrieving the Artius from the field, remove dirt from the bottom grooves using a stiff nylon brush or similar tool to ensure no mud or dirt is left. Inserting the device into the docking station with dirt might cause damage.




## 8. Appendices

### 8.1. Connector Pin-Outs

This is a 4-pin M12 D-code Automation connector.

Pin	Function
1	Power +
2	RS232 transmit
3	Power -
4	RS232 receive
<b>Shielding</b>	Ground
5	Unconnected

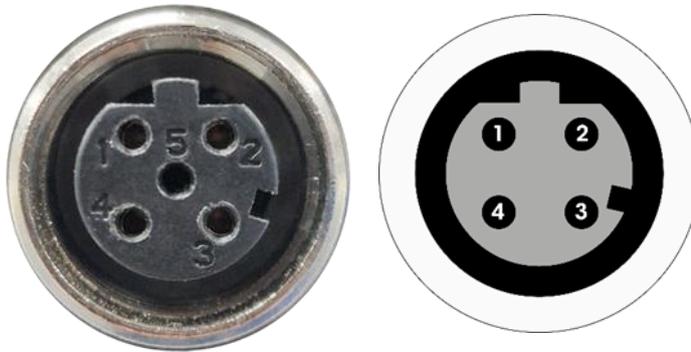

### 8.2. Network Ports

The following network ports are used by Artius:

Port	Layer 4 Protocol	Description
80	TCP	HTTP server
1565	TCP	GDI transmission protocol
1567	TCP/UDP	GCF transmission protocol
4242	TCP	File exchange protocol
4244	TCP	Remote console
11788	UDP	Remote procedure calls
18000	TCP	SEED-link transmission protocol
8190	TCP	Tunnel connection to server
7190	TCP	Tunnel Discovery to server

## 8.3. Channel Names

The tables in this section are designed to inform users of the names and codes of the streamed and recorded channels present in the Artius. The first character of a miniSEED channel code represents the sample rate. The possible values are shown in the table below:

Code	Sample Rate
<b>F</b>	≥ 1000 Hz to < 5000 Hz
<b>C</b>	≥ 250 Hz to < 1000 Hz
<b>H</b>	≥ 80 Hz to < 250 Hz
<b>B</b>	≥ 10 Hz to < 80 Hz
<b>M</b>	> 1 to < 10
<b>L</b>	≈ 1

The “Live Stream Codes” of the seismic channels are postfixed with “0” or “1”. This notation distinguishes between the two different sample rates that is possible to select for each streamed channel. For example, the streams `InstZ_0` and `InstZ_1` carry digitisations of the same signal, differing only in the sample rate.

Only one sample rate is available for the recorded seismic channels.

Sensor	Comp.	Digital filter mode	Data streaming		Data recording	
			Live stream name	Live stream code	Data record name	Mini SEED channel code
Seismic channels	Vertical	Acausal	InstZ	InstZ_0	InstZ_sd	xHZ
			InstZ	InstZ_1		
		Causal	InstZ_eew	InstZ_eew_0	InstZ_eew_sd	xHZ
	North	Acausal	InstN	InstN_0	InstN_sd	xHN
			InstN	InstN_1		
		Causal	InstN_eew	InstN_eew_0	InstN_eew_sd	xHN
	East	Acausal	InstE	InstE_0	InstE_sd	xHE
			InstE	InstE_1		
		Causal	InstE_eew	InstE_eew_0	InstE_eew_sd	xHE
Mass position channels	Vertical	Acausal	MassZ	MassZ_0	MassZ_sd	xMZ
	North	Acausal	MassN	MassN_0	MassN_sd	xMN
	East	Acausal	MassE	MassE_0	MassE_sd	xME
MEMS accelerometer	Vertical	Acausal	AccelZ	AccelZ_	AccelZ_sd	xNZ
	North	Acausal	AccelN	AccelN_	AccelN_sd	xNN
	East	Acausal	AccelE	AccelE_	AccelE_sd	xNE
Calibration channel		Acausal	Calibration	Calibration_0	Calibration_sd	xC0
Temperature		Acausal	Temperatur	Temperatur_0	Temperatur_sd	xKT

Sensor	Comp.	Data streaming			Data recording	
		Digital filter mode	Live stream name	Live stream code	Data record name	Mini SEED channel code
Input voltage		Acausal	S0Voltage	0VINP0	Voltage_sd	xQV
Power usage		Acausal	S0Power	0PINP0	Power_sd	xYP
Relative humidity		Acausal	Humidity	Humidity_0	Humidity_sd	xIH
NTP channels	Phase	Acausal	NTP_DAC_	NTP_DAC_	NTP_DAC_sd	LYT
	DAC	Acausal	NTP_Phase_	NTP_Phase_	NTP_Phase_sd	LYD
	Lpf	Acausal	NTP_lpf_	NTP_lpf_	NTP_lpf_sd	LYU
	Hpf	Acausal	NTP_hpf_	NTP_hpf_	NTP_hpf_sd	LYV
Internal Clock	PLL lock phase	Acausal	Phase_	Phase_	Phase_sd	LYP
	DAC	Acausal	DAC_	DAC_	DAC_sd	LQD
Battery pack	Voltage	Acausal	BattVoltage_	BattVoltage_	BattVoltage_sd	LQV
	Current	Acausal	BattCurrent_	BattCurrent_	BattCurrent_sd	LYI
	Charge Volts	Acausal	BattChargeV_	BattChargeV_	BattChargeV_sd	LQQ
	Charge current	Acausal	BattChargeI_	BattChargeI_	BattChargeI_sd	LYQ
	Temperature	Acausal	BattTemp_	BattTemp_	BattTemp_sd	LYT
	Charge	Acausal	BattCharge_	BattCharge_	BattCharge_sd	LYC
	Power	Acausal	BatteryPower_	BatteryPower	BatteryPower_sd	LYW

